

Independent Clinical Study Results



STUDY SCOPE


30 female volunteers aged between 35-65 took part in a home-use study conducted by Aspen Clinical Research to test the efficacy of the CACI Microlift anti-ageing device. The CACI Microlift was used by the volunteers for 10 minutes, 3 times per week over a 4 week period (2 hours total usage).

THE RESULTS

WRINKLE DEPTH REDUCED

By over **1/3** after just 4 weeks


REDUCTION IN FINE LINES & WRINKLES

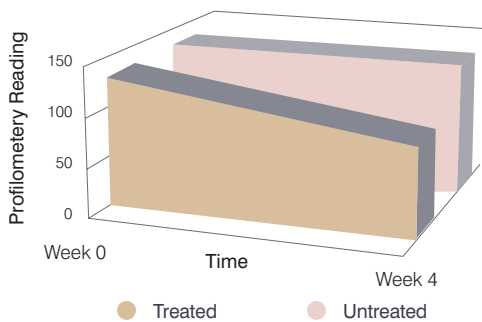

SKIN ELASTICITY IMPROVED

Up to **38%** after just 4 weeks

MEASUREMENT OF SKIN ELASTICITY

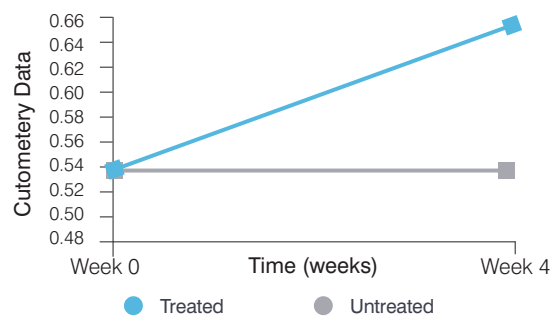

STUDY VOLUNTEER OBSERVATIONS

SKIN IMPROVED

83%

FINE LINES SOFTENED

77%

SKIN LOOKED MORE TONED

80%

FIRMER SKIN

77%

LIFTED FACIAL CONTOURS


80%

SKIN MORE SUPPLE

73%


PERSONAL FACIAL TONING SYSTEM

Would you continue using this device as part of your regular skin care routine?

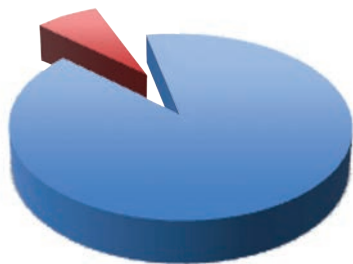

93% Yes 7% No

Do you believe if you used this device regularly it would contribute to your age management skin programme?

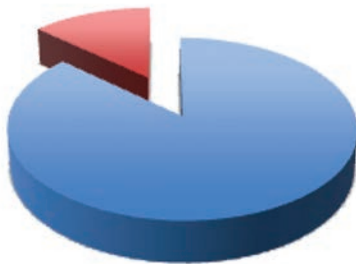


87% Yes 13% No

What other changes did you notice in the appearance / feel of the skin on your face?



More toned
Firmer
Younger looking
Reduced fine lines
General Improvement
Reduced wrinkles / deep wrinkles

RESULTS AFTER JUST 4 WEEKS USAGE



Patented Muscle Gripping Action

Protected by European Community Patents 1964008-0001; 29/408 800. International Patents Pending 1014274.3; 12/870,361.



CACI
— microlift —

CACI Microlift Ltd
514, Centennial Avenue, Centennial Park,
Elstree Hertfordshire WD6 3FG
0845 208 0268 www.cacimicrolift.com