

# Independent Clinical Study Results



## STUDY SCOPE


30 female volunteers aged between 35-65 took part in a home-use study conducted by Aspen Clinical Research to test the efficacy of the CACI Microlift anti-ageing device. The CACI Microlift was used by the volunteers for 10 minutes, 3 times per week over a 4 week period (2 hours total usage).

## THE RESULTS

### WRINKLE DEPTH REDUCED

By over **1/3** after just 4 weeks


REDUCTION IN FINE LINES & WRINKLES

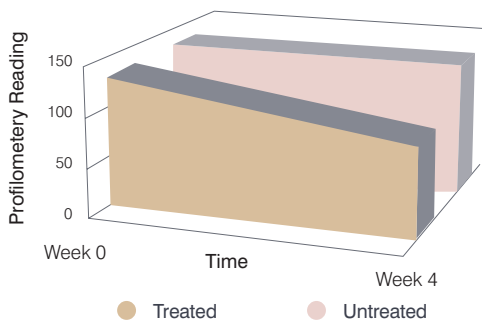

### SKIN ELASTICITY IMPROVED

Up to **38%** after just 4 weeks

MEASUREMENT OF SKIN ELASTICITY

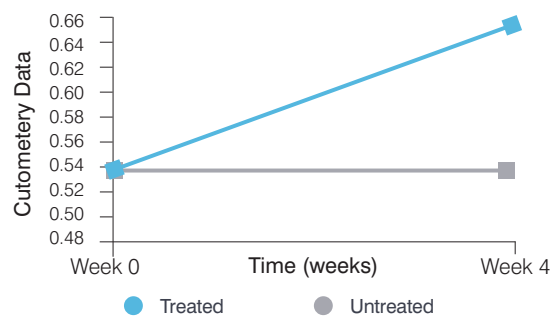

## STUDY VOLUNTEER OBSERVATIONS

SKIN IMPROVED

**83%**

FINE LINES SOFTENED

**77%**

SKIN LOOKED MORE TONED

**80%**

FIRMER SKIN

**77%**

LIFTED FACIAL CONTOURS


**80%**

SKIN MORE SUPPLE

**73%**


PERSONAL FACIAL TONING SYSTEM

Would you continue using this device as part of your regular skin care routine?

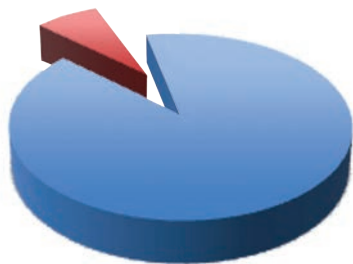

93% Yes 7% No

Do you believe if you used this device regularly it would contribute to your age management skin programme?

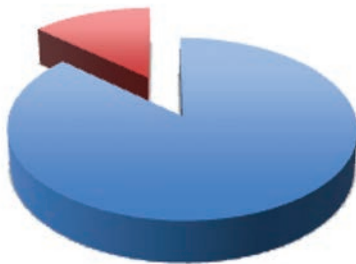


87% Yes 13% No

What other changes did you notice in the appearance / feel of the skin on your face?



● More toned  
● Fimer  
● Younger looking  
● Reduced fine lines  
● General Improvement  
● Reduced wrinkles / deep wrinkles

## RESULTS AFTER JUST 4 WEEKS USAGE



**Patented Muscle Gripping Action**

Protected by European Community Patents 1964008-0001; 29/408 800. International Patents Pending 1014274.3; 12/870,361.

